



# UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE  
United States Patent and Trademark Office  
Address: COMMISSIONER FOR PATENTS  
P.O. Box 1450  
Alexandria, Virginia 22313-1450  
www.uspto.gov

APPLICATION NO.	FILING DATE	FIRST NAMED INVENTOR	ATTORNEY DOCKET NO.	CONFIRMATION NO.
-----------------	-------------	----------------------	---------------------	------------------

10/785,672

02/23/2004

Michael P. Whitman

11443/160

2683

26646

7590

02/01/2007

KENYON & KENYON LLP  
ONE BROADWAY  
NEW YORK, NY 10004

EXAMINER

WEEKS, GLORIA R

ART UNIT

PAPER NUMBER

3721

SHORTENED STATUTORY PERIOD OF RESPONSE	MAIL DATE	DELIVERY MODE
--	-----------	---------------

3 MONTHS

02/01/2007

PAPER

**Please find below and/or attached an Office communication concerning this application or proceeding.**

If NO period for reply is specified above, the maximum statutory period will apply and will expire 6 MONTHS from the mailing date of this communication.

88

<b>Office Action Summary</b>	<b>Application No.</b> 10/785,672	<b>Applicant(s)</b> WHITMAN ET AL.	
	<b>Examiner</b> Gloria R. Weeks	<b>Art Unit</b> 3721	

-- The MAILING DATE of this communication appears on the cover sheet with the correspondence address --  
**Period for Reply**

A SHORTENED STATUTORY PERIOD FOR REPLY IS SET TO EXPIRE 3 MONTH(S) OR THIRTY (30) DAYS, WHICHEVER IS LONGER, FROM THE MAILING DATE OF THIS COMMUNICATION.

- Extensions of time may be available under the provisions of 37 CFR 1.136(a). In no event, however, may a reply be timely filed after SIX (6) MONTHS from the mailing date of this communication.
- If NO period for reply is specified above, the maximum statutory period will apply and will expire SIX (6) MONTHS from the mailing date of this communication.
- Failure to reply within the set or extended period for reply will, by statute, cause the application to become ABANDONED (35 U.S.C. § 133). Any reply received by the Office later than three months after the mailing date of this communication, even if timely filed, may reduce any earned patent term adjustment. See 37 CFR 1.704(b).

**Status**

- 1) ☒ Responsive to communication(s) filed on 16 January 2007.
- 2a) ☐ This action is **FINAL**.                      2b) ☒ This action is non-final.
- 3) ☐ Since this application is in condition for allowance except for formal matters, prosecution as to the merits is closed in accordance with the practice under *Ex parte Quayle*, 1935 C.D. 11, 453 O.G. 213.

**Disposition of Claims**

- 4) ☒ Claim(s) 100-106 is/are pending in the application.
- 4a) Of the above claim(s) \_\_\_\_\_ is/are withdrawn from consideration.
- 5) ☐ Claim(s) \_\_\_\_\_ is/are allowed.
- 6) ☒ Claim(s) 100-106 is/are rejected.
- 7) ☐ Claim(s) \_\_\_\_\_ is/are objected to.
- 8) ☐ Claim(s) \_\_\_\_\_ are subject to restriction and/or election requirement.

**Application Papers**

- 9) ☐ The specification is objected to by the Examiner.
- 10) ☐ The drawing(s) filed on \_\_\_\_\_ is/are: a) ☐ accepted or b) ☐ objected to by the Examiner.  
 Applicant may not request that any objection to the drawing(s) be held in abeyance. See 37 CFR 1.85(a).  
 Replacement drawing sheet(s) including the correction is required if the drawing(s) is objected to. See 37 CFR 1.121(d).
- 11) ☐ The oath or declaration is objected to by the Examiner. Note the attached Office Action or form PTO-152.

**Priority under 35 U.S.C. § 119**

- 12) ☐ Acknowledgment is made of a claim for foreign priority under 35 U.S.C. § 119(a)-(d) or (f).
- a) ☐ All    b) ☐ Some \* c) ☐ None of:
1. ☐ Certified copies of the priority documents have been received.
2. ☐ Certified copies of the priority documents have been received in Application No. \_\_\_\_\_.
3. ☐ Copies of the certified copies of the priority documents have been received in this National Stage application from the International Bureau (PCT Rule 17.2(a)).
- \* See the attached detailed Office action for a list of the certified copies not received.

**Attachment(s)**

- |  |   |
|--|---|
| 1) <input type="checkbox"/> Notice of References Cited (PTO-892)   | 4) <input type="checkbox"/> Interview Summary (PTO-413)<br>Paper No(s)/Mail Date. _____ |
| 2) <input type="checkbox"/> Notice of Draftsperson's Patent Drawing Review (PTO-948)                                   | 5) <input type="checkbox"/> Notice of Informal Patent Application (PTO-152)             |
| 3) <input type="checkbox"/> Information Disclosure Statement(s) (PTO-1449 or PTO/SB/08)<br>Paper No(s)/Mail Date _____ | 6) <input type="checkbox"/> Other: _____  |

***Continued Examination Under 37 CFR 1.114***

1. A request for continued examination under 37 CFR 1.114, including the fee set forth in 37 CFR 1.17(e), was filed in this application after final rejection. Since this application is eligible for continued examination under 37 CFR 1.114, and the fee set forth in 37 CFR 1.17(e) has been timely paid, the finality of the previous Office action has been withdrawn pursuant to 37 CFR 1.114. Applicant's submission filed on January 16, 2007 has been entered.

***Claim Rejections - 35 USC § 102***

2. The following is a quotation of the appropriate paragraphs of 35 U.S.C. 102 that form the basis for the rejections under this section made in this Office action:

A person shall be entitled to a patent unless –

(b) the invention was patented or described in a printed publication in this or a foreign country or in public use or on sale in this country, more than one year prior to the date of application for patent in the United States.

3. Claims 100-103 are rejected under 35 U.S.C. 102(b) as being anticipated by Grant et al. (USPN 5,609,285).

In reference to claims 100-103, Grant et al. discloses a surgical device, comprising: a staple housing (70) defining a bore; a trocar shaft (84) disposed through the bore of the housing (70; figure 7) so as to be moveable relative to the housing (70) by operation of at least one driver (82) within the housing, wherein at least a portion of the trocar shaft (84) is flexible; and an anvil (100) attachable to the trocar shaft (84) and configured to be moveable relative to the housing (70) by movement of the trocar shaft (84; column 11 lines 1-35; column 14 lines 14-18), wherein the anvil (100) includes an anvil shaft (110), the anvil shaft defining a trocar receiving slot, and the trocar shaft (84) including a trocar (200) configured to be insertable within the trocar receiving slot (figure 38); and the trocar receiving slot is defined in an anvil sleeve having an

Art Unit: 3721

axially-extending bore in communication with the trocar receiving slot, wherein the axially-extending bore has a wide portion into which the trocar (200) is insertable and a narrow portion (435) which retains the trocar within the axially-extending bore.

***Claim Rejections - 35 USC § 103***

4. The following is a quotation of 35 U.S.C. 103(a) which forms the basis for all obviousness rejections set forth in this Office action:

(a) A patent may not be obtained though the invention is not identically disclosed or described as set forth in section 102 of this title, if the differences between the subject matter sought to be patented and the prior art are such that the subject matter as a whole would have been obvious at the time the invention was made to a person having ordinary skill in the art to which said subject matter pertains. Patentability shall not be negated by the manner in which the invention was made.

5. Claims 104-106 are rejected under 35 U.S.C. 103(a) as being obvious over Grant et al. (USPN 5,609,285) in view of Whitman (USPN 6,491,201).


Regarding claims 104-106, Grant et al. discloses a surgical instrument having a driver, but does not disclose the driver as being rotatable via an operator controlled motor. Whitman teaches a surgical instrument having a flexible shaft (215) movable relative to a housing (155) by way of a rotatable driver (170) selectively rotated by at least one motor (165) via a controller (160). It would have been obvious to one having ordinary skill in the art at the time of the invention to modify the surgical instrument of Grant et al. to include the motor rotatable driver of Whitman, as column 3 lines 17-31 of Whitman states that such a modification allows an operator to selectively alter the direction in which the driver shaft is rotated.

***Response to Arguments***

6. Applicant's arguments filed January 16, 2007 have been fully considered but they are not persuasive.


Art Unit: 3721

Applicant has first argued that Grant et al. fails to disclose a flexible portion of a trocar shaft extending distally relative to a distal end of a housing. Examiner has interpreted the term distal to be defined as anatomically located far from a point of reference, such as an origin or a point of attachment.<sup>1</sup> The origin defined in claim 100 is the distal end of the staple housing, however, no reference is made to the point of origin that defines the end of the staple housing that is deemed distal. Thus, broadly interpreted, examiner has found the distal end of the housing 104 to be the end engaging spring 152, therefore, a distal direction from this point of engagement would be towards the anvil 100. Therefore, Grant et al. is found to disclose the invention as claimed, since figure 7 (*see diagram below*) illustrates the a flexible portion 84 of the trocar shaft to extend distally from the distal end of the housing 70, as interpreted above.

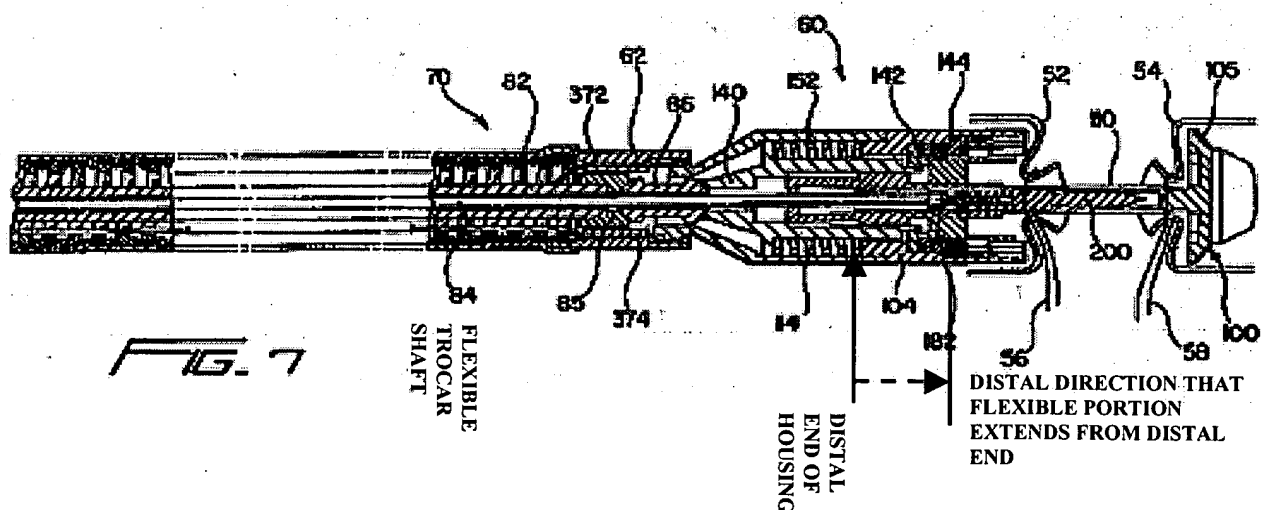

Nonetheless, even if one were to interpret the distal end of the housing to be opposite to the distal end illustrated above, one could still find Grant et al. to disclose the limitations of Applicants invention as claimed, per the illustration below.

<sup>1</sup> American Heritage Dictionary

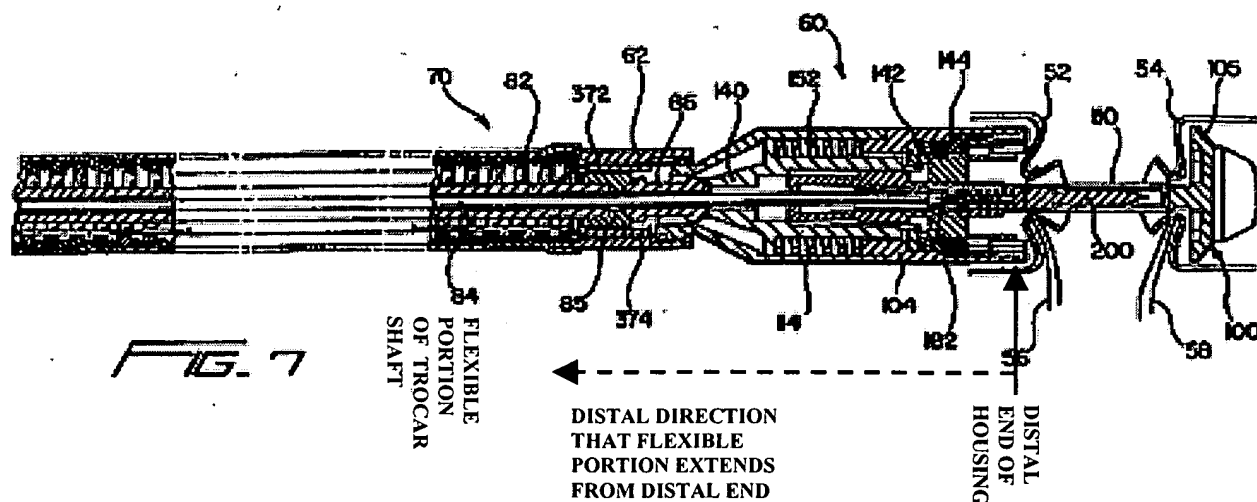

### Conclusion

7. Any inquiry concerning this communication or earlier communications from the examiner should be directed to Gloria R. Weeks whose telephone number is (571) 272-4473.

The examiner can normally be reached on M-F 8am-4pm.

If attempts to reach the examiner by telephone are unsuccessful, the examiner's supervisor, Rinaldi I. Rada can be reached on (571) 272-4467. The fax phone number for the organization where this application or proceeding is assigned is 571-273-8300.

Information regarding the status of an application may be obtained from the Patent Application Information Retrieval (PAIR) system. Status information for published applications may be obtained from either Private PAIR or Public PAIR. Status information for unpublished applications is available through Private PAIR only. For more information about the PAIR system, see <http://pair-direct.uspto.gov>. Should you have questions on access to the Private PAIR system, contact the Electronic Business Center (EBC) at 866-217-9197 (toll-free).

Art Unit: 3721


Other helpful telephone numbers are listed for applicant's benefit:

- Allowed Files & Publication (888) 786-0101
- Assignment Branch (800) 972-6382
- Certificates of Correction (703) 305-8309
- Fee Questions (571) 272-6400
- Inventor Assistance Center (800) PTO-9199
- Petitions/special Programs (571) 272-3282
- Information Help line 1-800-786-9199

grw

January 25, 2007

Gloria R. Weeks  
Examiner  
Art Unit 3721

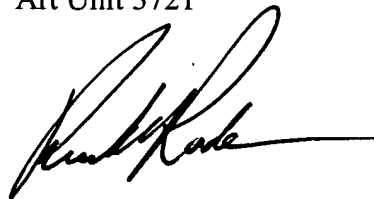

Rinaldi I. Rada  
Supervisory Patent Examiner  
Group 3700